

AirFit™ N30i P30i



This is for the active sleepers,
who go to bed when it suits them.
For the night-time nomads
who twist and turn
then spring up to take on the day.



Freedom to move


The ResMed AirFit N30i and AirFit P30i give your patients the freedom to sleep in any position and get close to their bed partner. Both masks feature the same discreet, minimalist design with a convenient top-of-the-head tube and a self-adjusting SpringFit frame for a stable fit that lasts all night.^{1,2}



Respond to wants as well as needs

The tube-up design of the N30i and P30i is designed to let patients sleep in any position without compromising seal or comfort.

The snugly fitting SpringFit frame, carefully engineered cushions and tube-up design keep pace with every twist and turn. If your patient gets up during the night, the quick-release elbow keeps life simple.

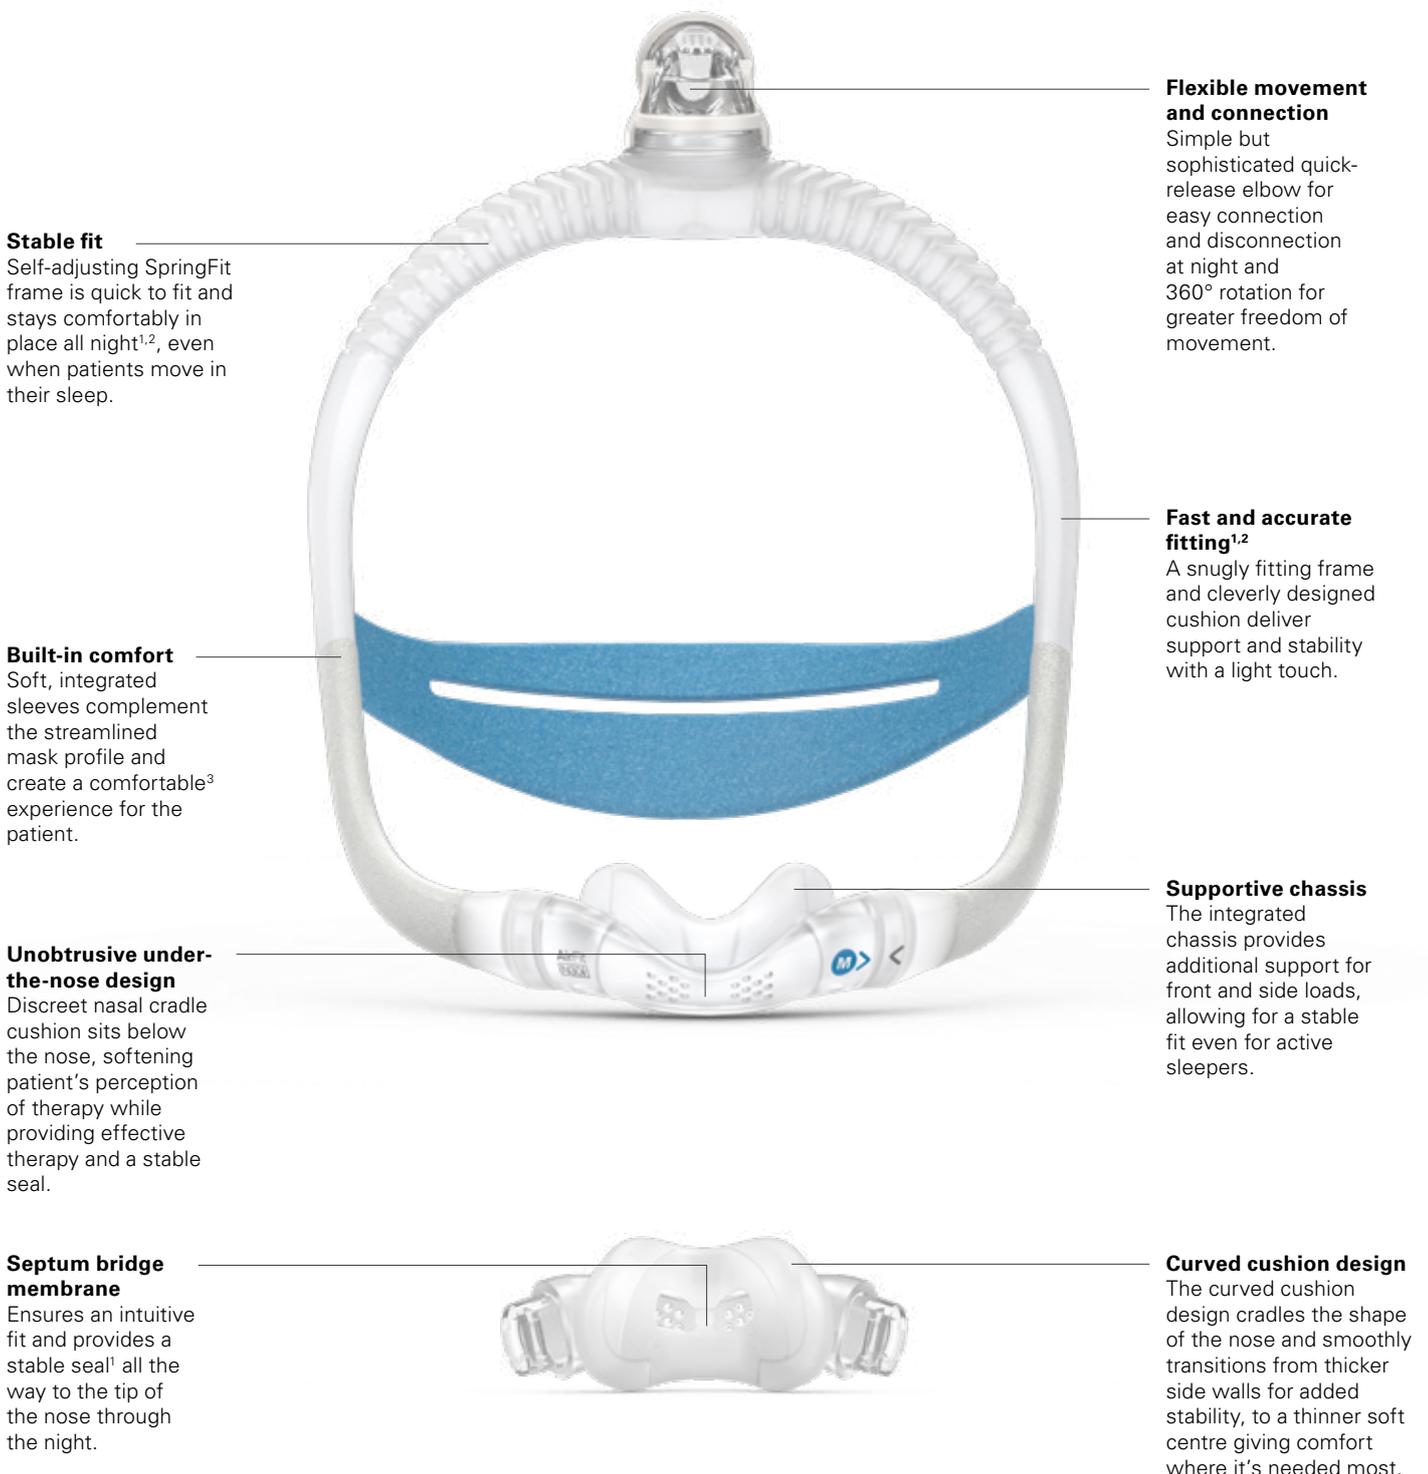



Offer freedom and flexibility. Maintain simplicity.

The modular, mix-and-match design of the AirFit N30i and AirFit P30i means you can do more with less. Offer patients the freedom of an ultra-compact tube-up mask. Let them choose a pillows mask if they prefer. Switch easily between nasal cradle and pillows cushions when you need to alter the seal or change contact points. Mix-and-match makes it quick and simple to offer your patients more freedom and greater flexibility.



QuietAir vent

Exhaled air is gently diffused to limit noise output.² This whisper-quiet, wovenmesh vent emits just 21 dBA⁴ for a more relaxing environment in the bedroom.



Dual-wall technology performs a dual function, promoting comfort while creating a reliable seal.² The cushion seals on contact and air is released gently.



Streamline your business

The AirFit N30i and AirFit P30i share the same streamlined, modular design to minimise fitting time and facilitate stock management. There are just two frame sizes and one size of headgear. Each mask has two cushion sizes that are designed to deliver a good fit for the vast majority of patients. To ensure there's an option for everyone, the N30i cushion is also available in wide and small wide versions and there's a large size for the P30i.

Only two starter packs for simplified stock management

AirFit N30i Small starter pack (63816)

Provided in this pack:

- AirFit N30i small frame
- Headgear
- Cushions: S, M

AirFit P30i Small starter pack (63866)

Provided in this pack:

- AirFit P30i small frame
- Headgear
- Cushions: S, M



AirFit N30i Standard starter pack (63815)


Provided in this pack:

- AirFit N30i standard frame
- Headgear
- Cushions: S, M

AirFit P30i Standard starter pack (63865)

Provided in this pack:

- AirFit P30i standard frame
- Headgear
- Cushions: S, M

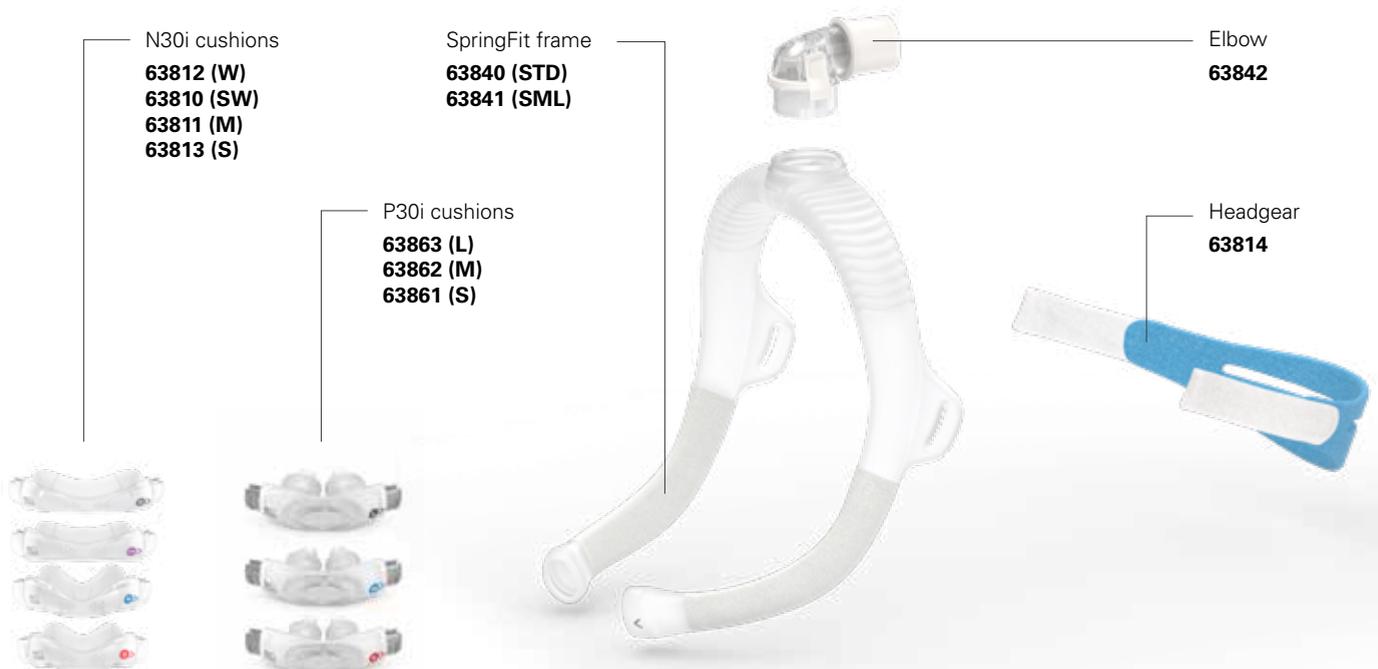

AirFit™ N30i

AirFit™ P30i



Nasal cradle mask



Nasal pillows mask

Fitting guide



- Pull the frame and headgear over your head until the elbow is positioned on top and the headgear is behind your head.



- Place the cushion under your nose.
- For the AirFit P30i mask, align the pillows into your nostrils.



- Tighten or loosen the headgear until the cushion fits comfortably under your nose.



- Squeeze the side buttons on the elbow and detach from the frame.



- Connect the air tubing from your device to the elbow.




- Reattach the elbow to the frame.
- The mask is now ready to use.

Refer to the user guide for further instructions.



Additional options

- For patients with longer hair, we recommend feeding their hair through the back of the headgear. If tied in a pony tail, it should sit high enough to fit comfortably through the back of the headgear.
- Refer to the user guide for further instructions and complete labeling information including indications, contraindications, warnings and precautions.

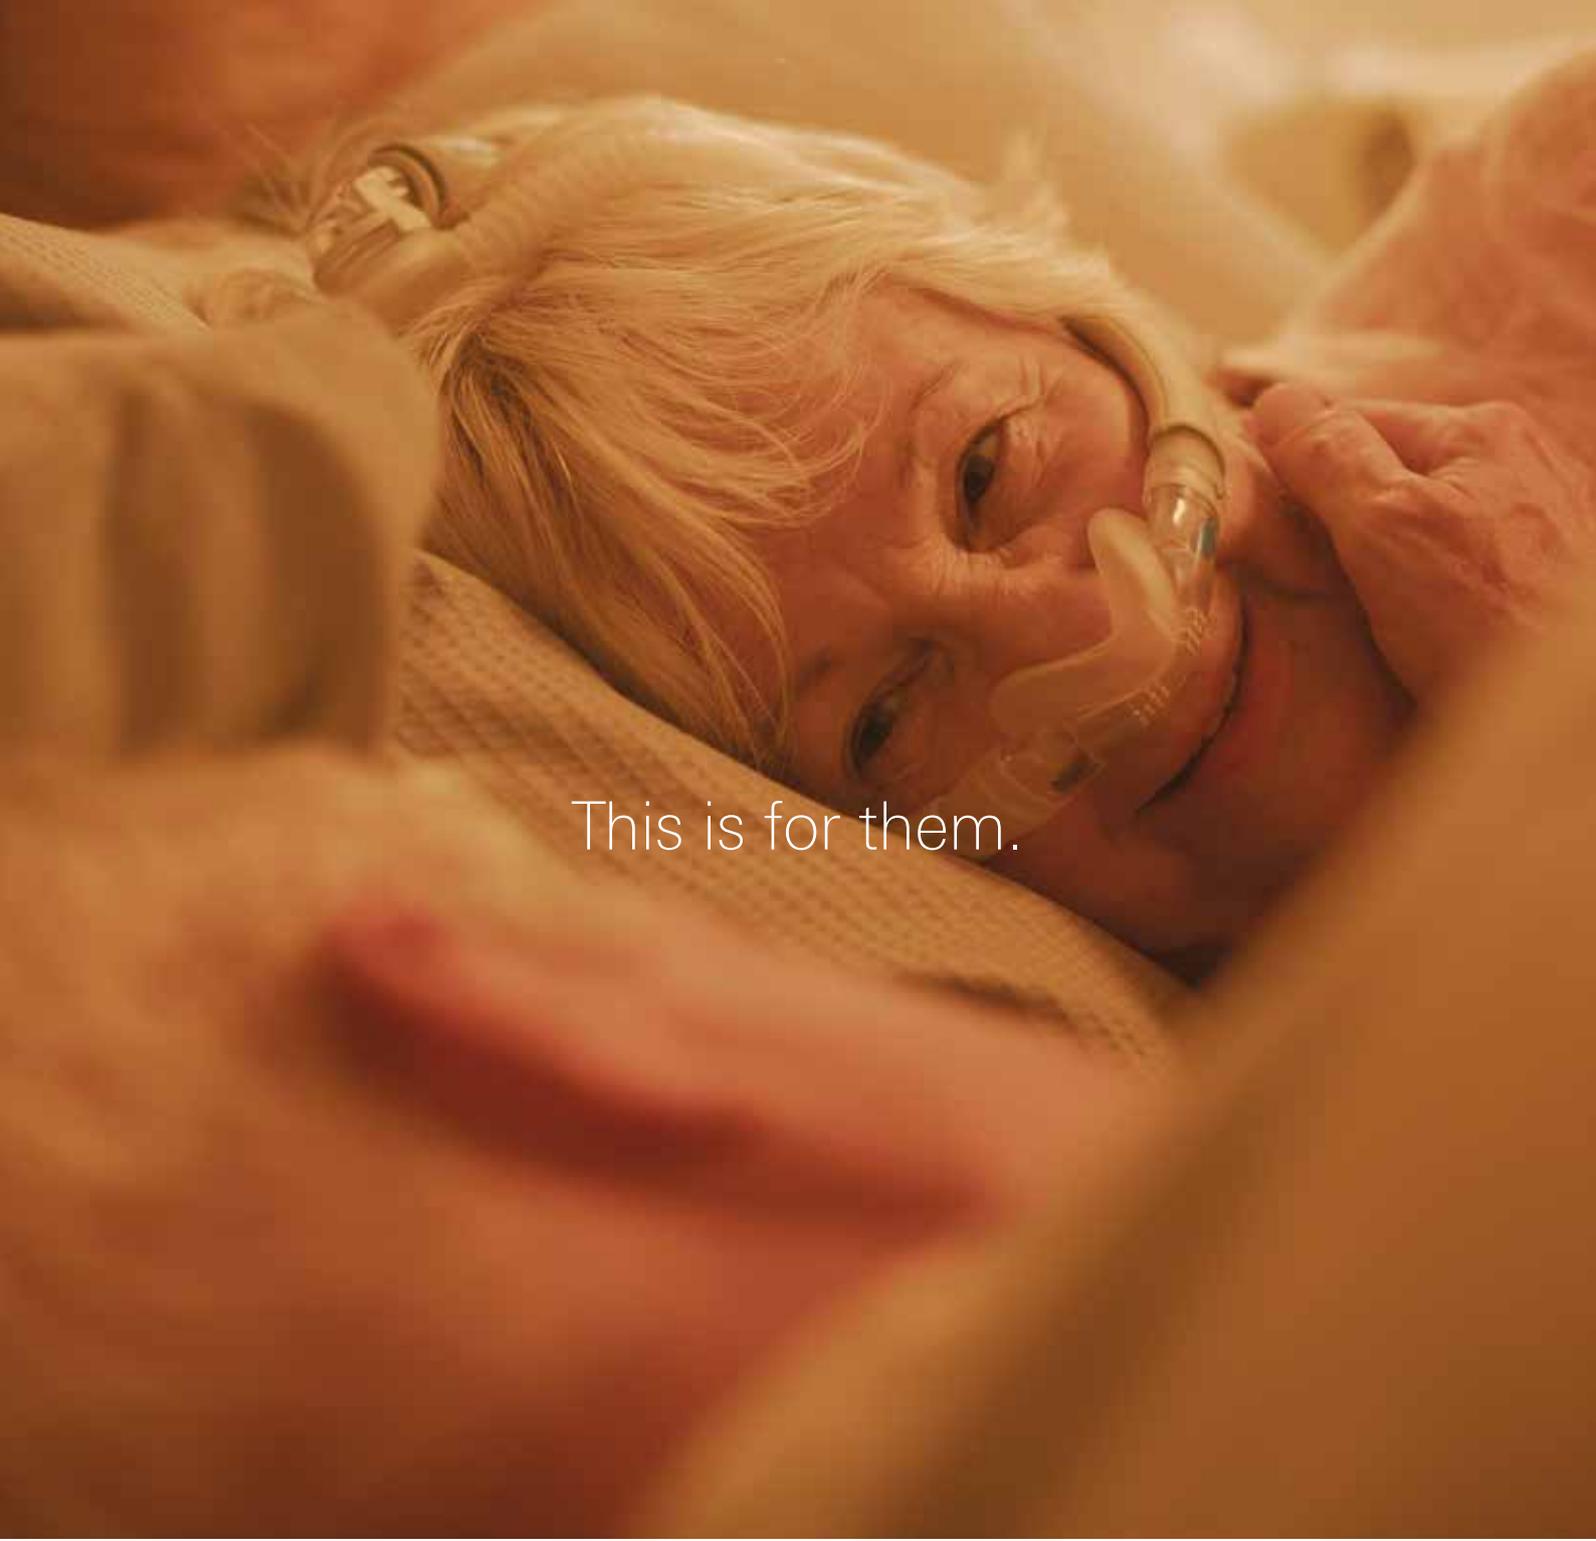

This is for them.

1 ResMed external 7-day clinical study of 24 ResMed and non-ResMed patients, conducted between 21/02/2018 - 12/03/2018. Data on file; ID A4320645.
2 ResMed external 14-day clinical study of 23 ResMed patients, conducted between 30/05/2018 - 22/06/2018. Data on file; ID A4387859.
3 ResMed external fitting study of existing 37 ResMed and non-ResMed patients, conducted between 09/04/2018 - 20/04/2018. Data on file; ID A4327753. 4 Sound power level of 21 dBA - AirFit P30i user guide, ResMed Pty Ltd 2018. ID A4461185.

AirFit, QuietAir and Air20 are trademarks of ResMed Pty Ltd.
Specifications may change without notice.
© 2019 ResMed. 10111212/1 2019-03

[ResMed.com /AirFit30](https://www.resmed.com/airfit30)